

Resusci Baby


for

First Aid

User Guide




Resusci Baby for First Aid

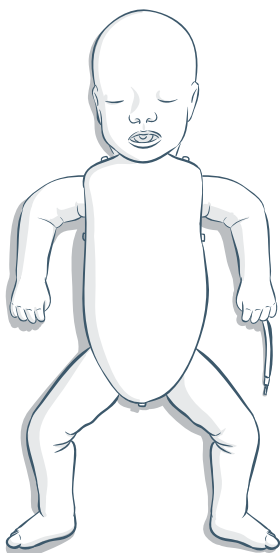

x 2



x 6



x 5





4




5





5














6












7

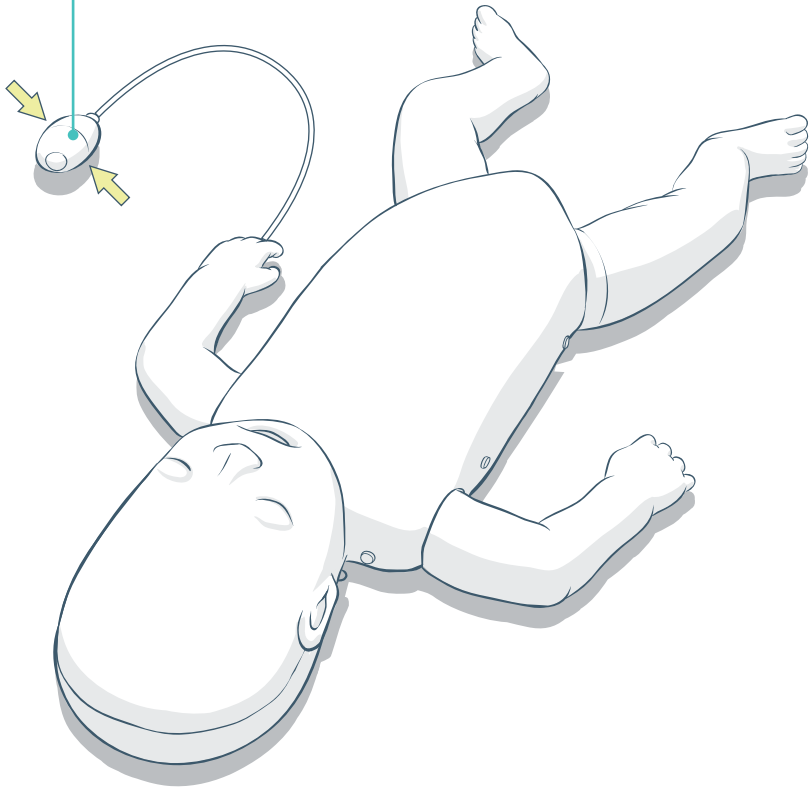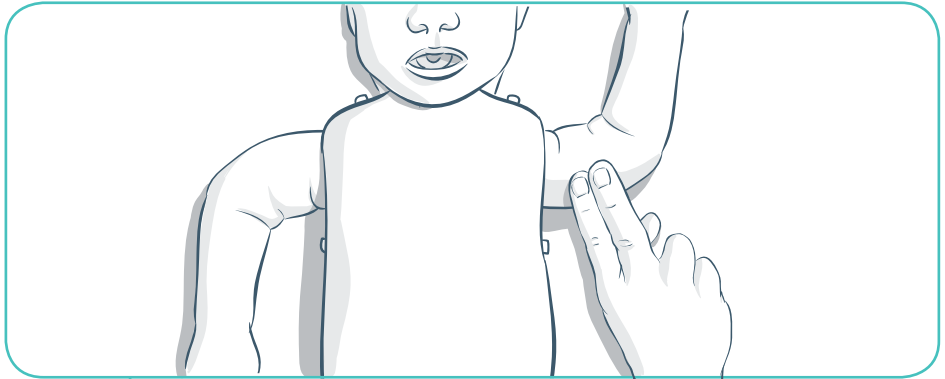

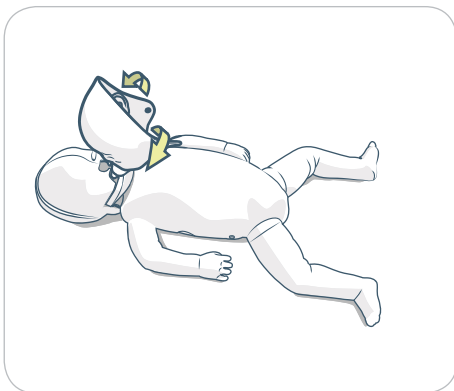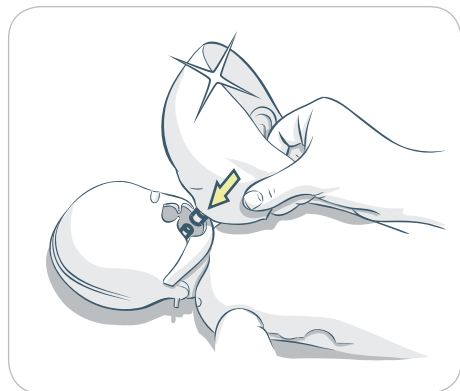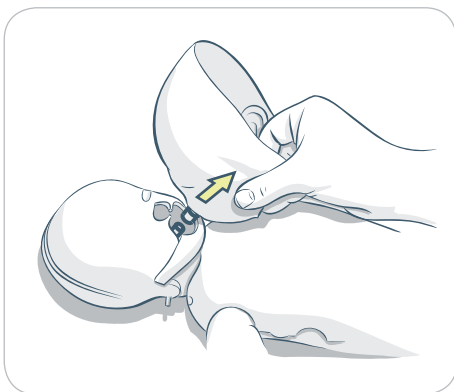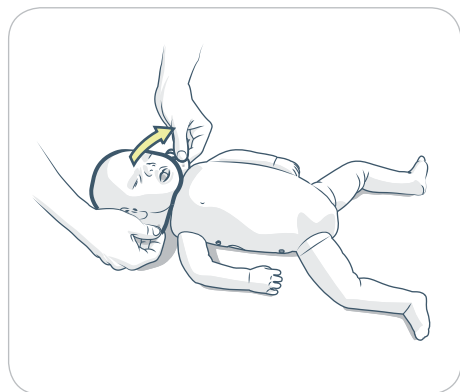

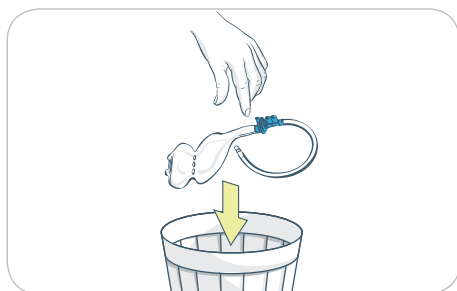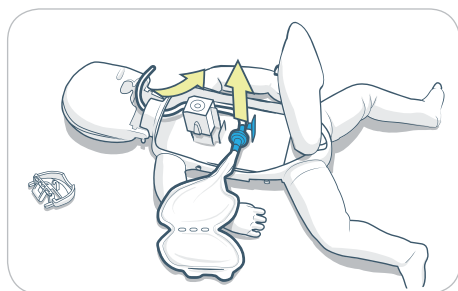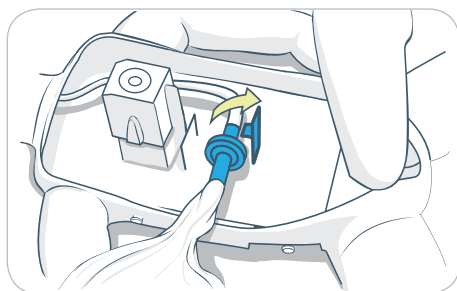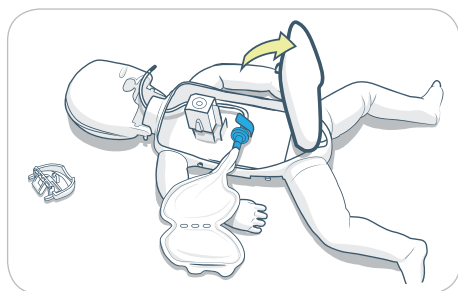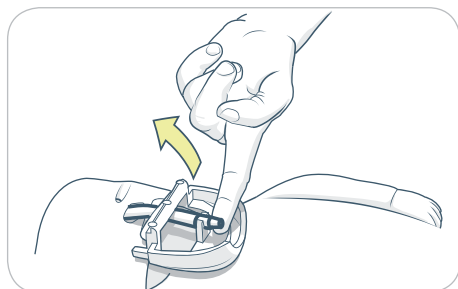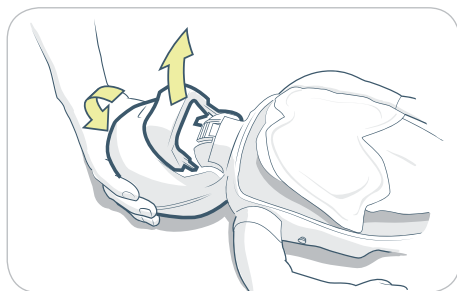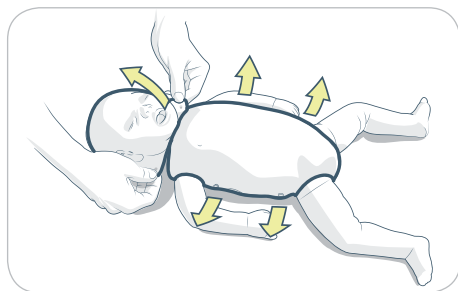

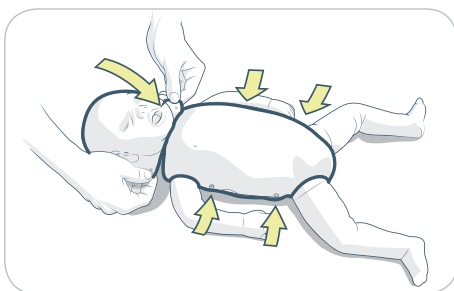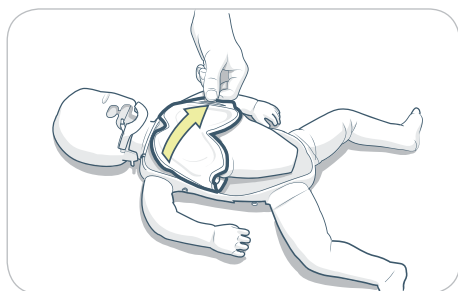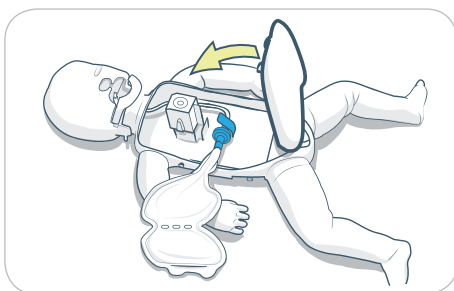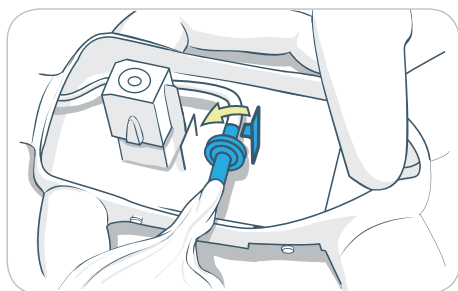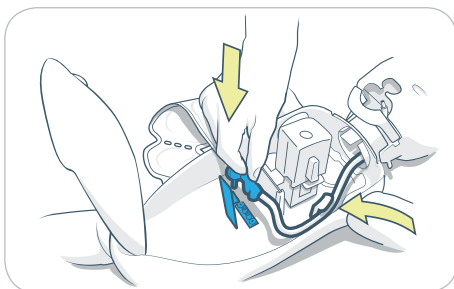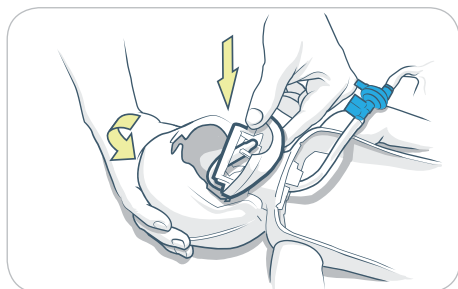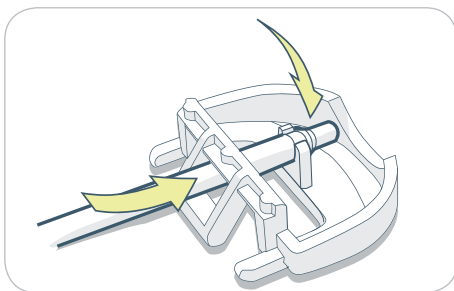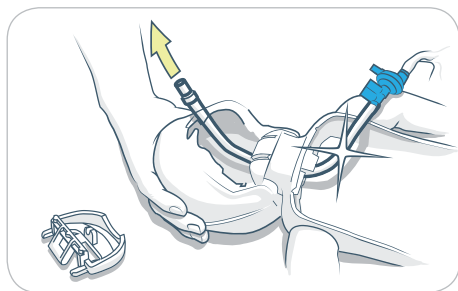

© 2013 Laerdal Medical AS. All rights reserved.
Device Manufacturer: Laerdal Medical AS, P.O. Box 377,
Tanke Svilandsgate 30, 4002 Stavanger, Norway
T: (+47) 5151 1700

20-05950 Rev A

