



Resusci Baby

with
QCPR

User Guide



Resusci Baby with QCPR

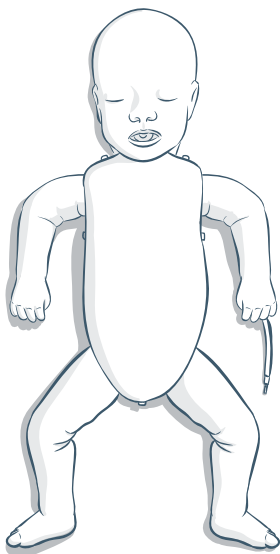



4




7



7



8





9










10













11





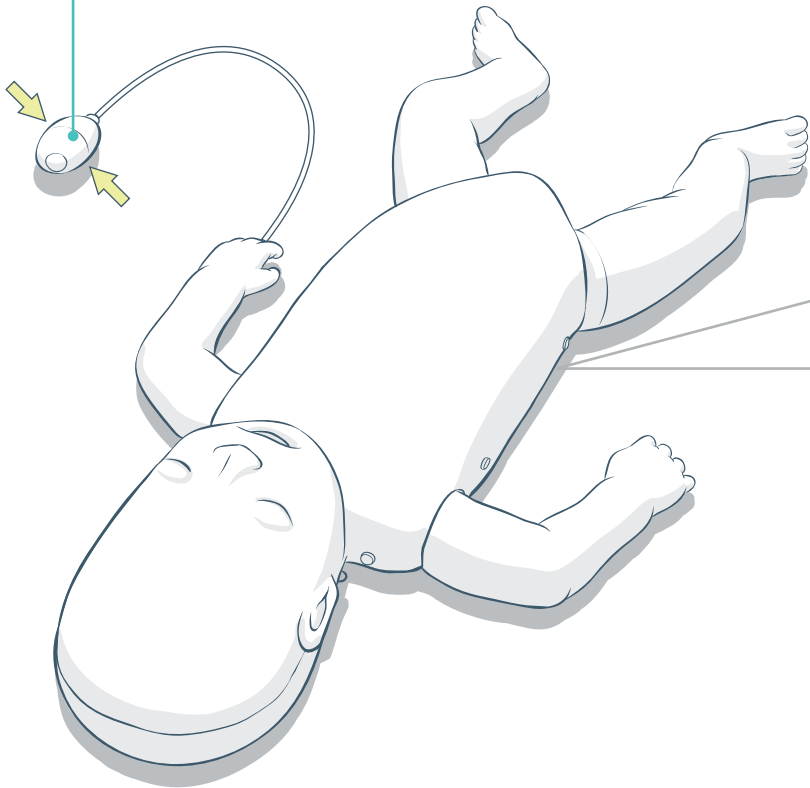
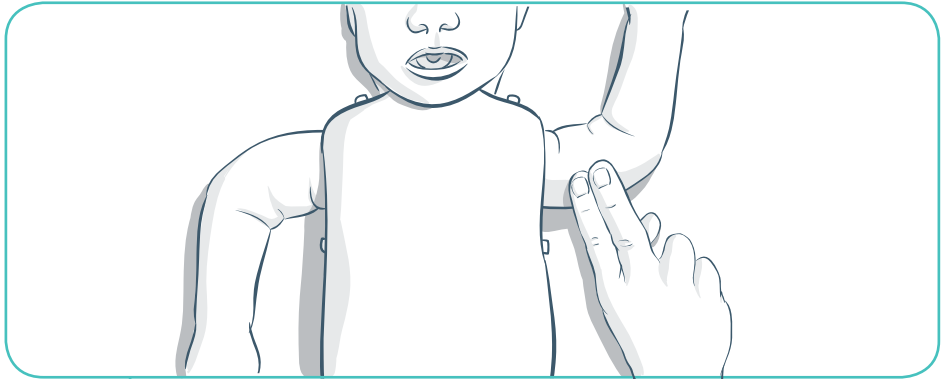





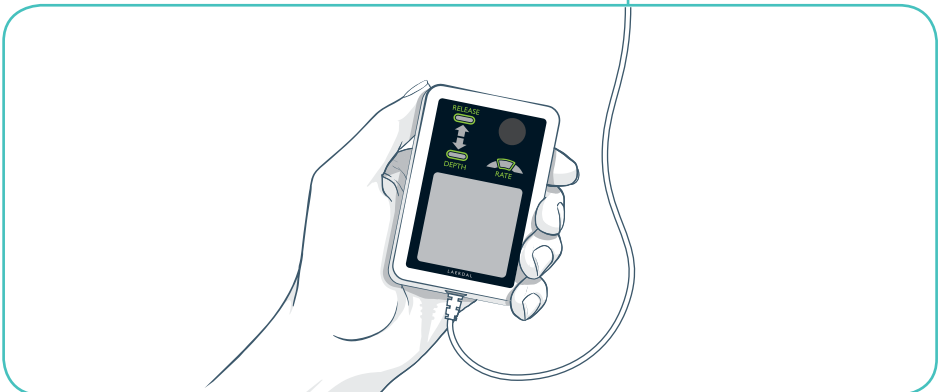
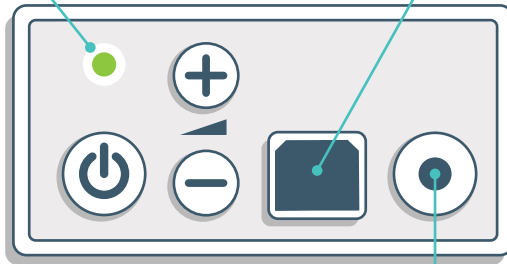
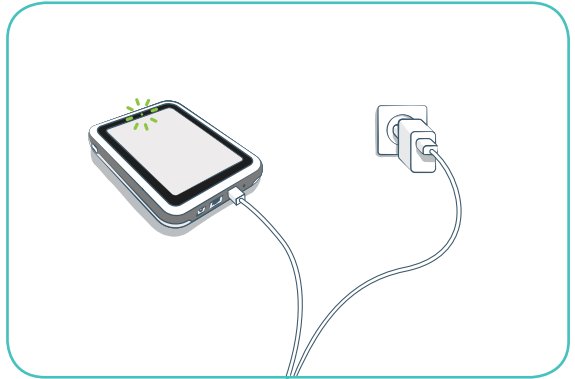
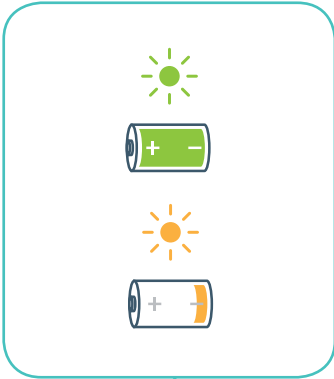








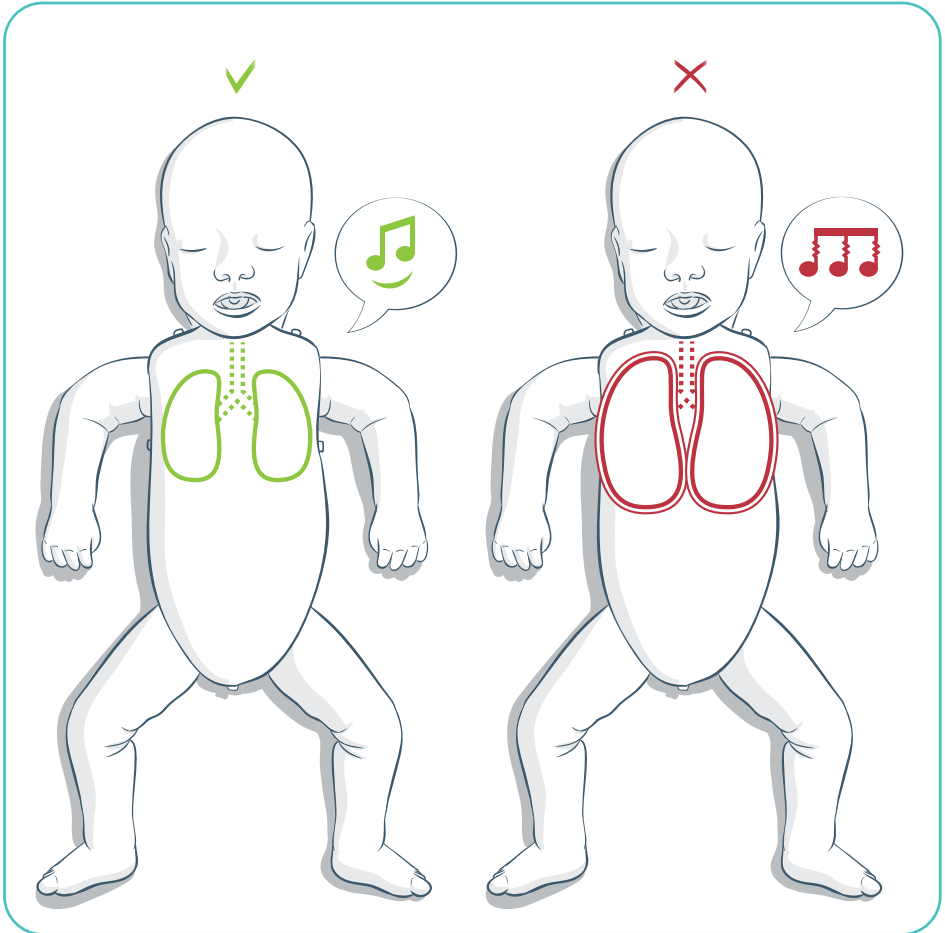
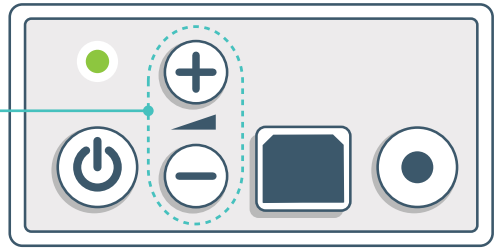
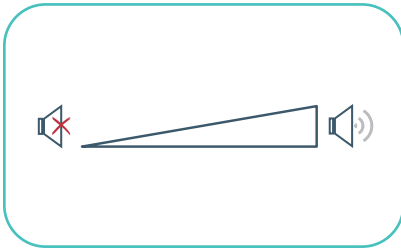


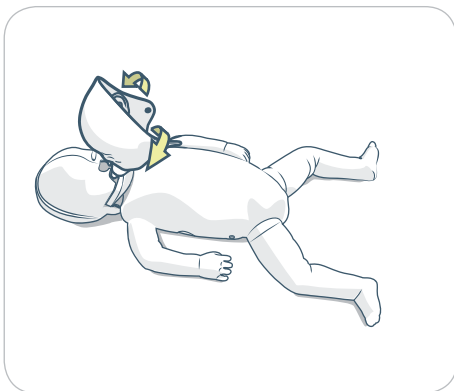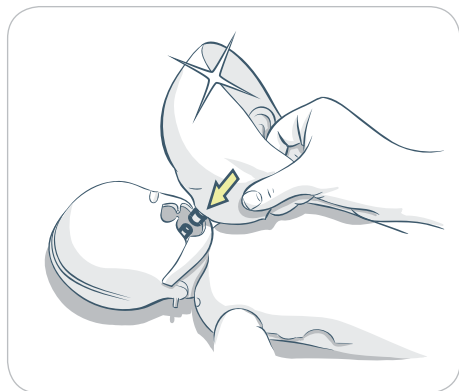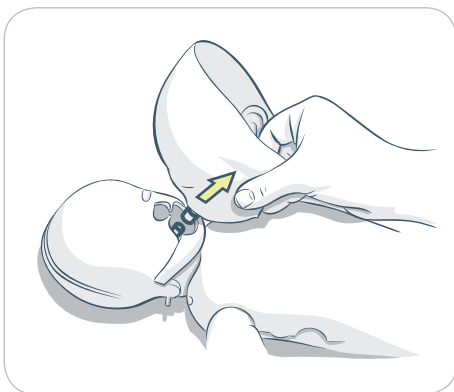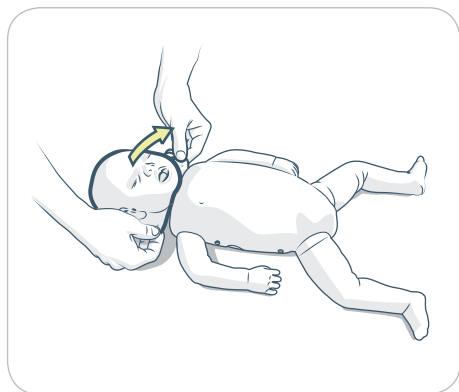

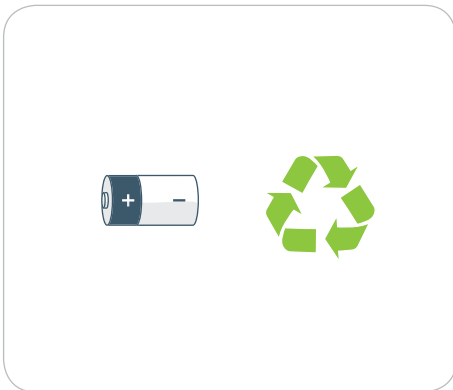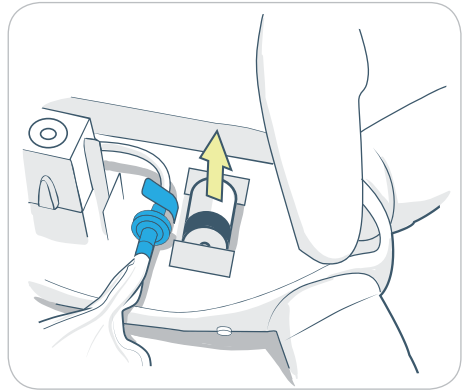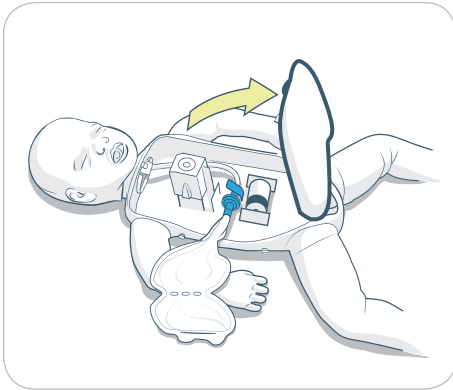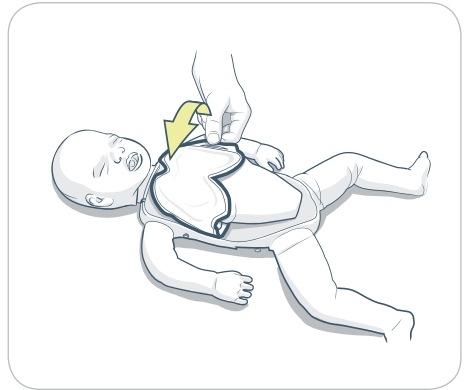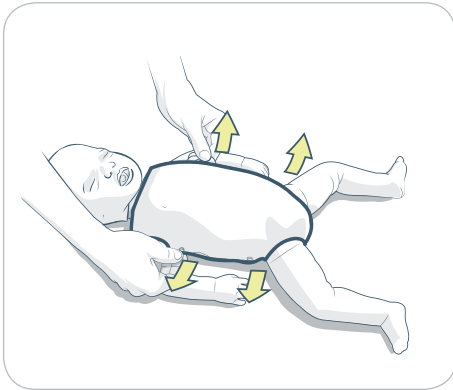

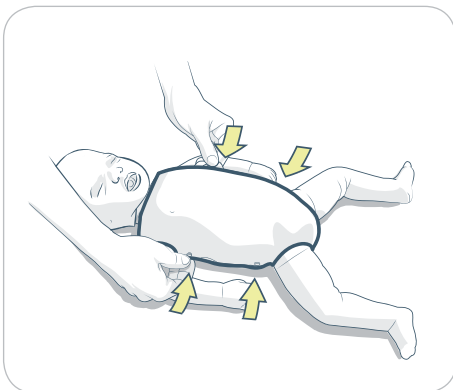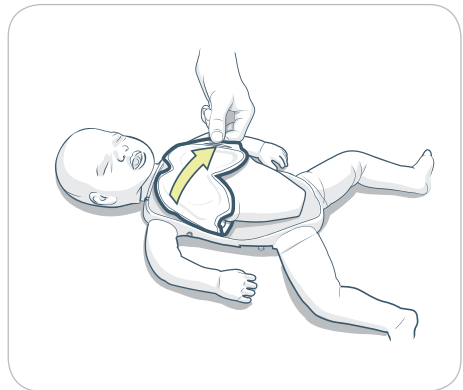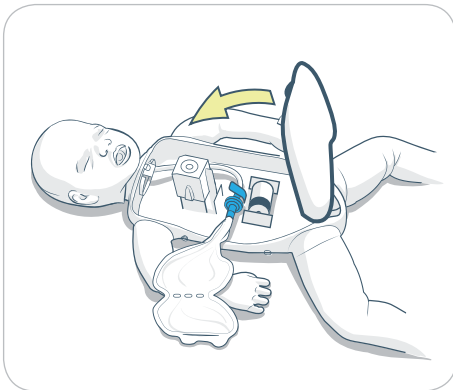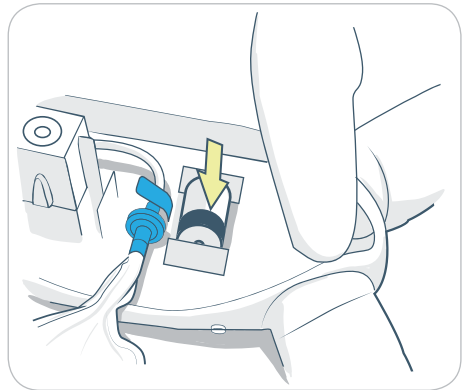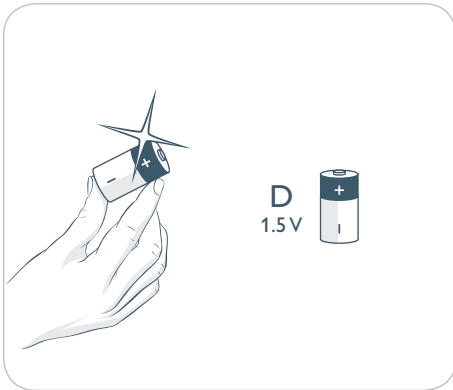

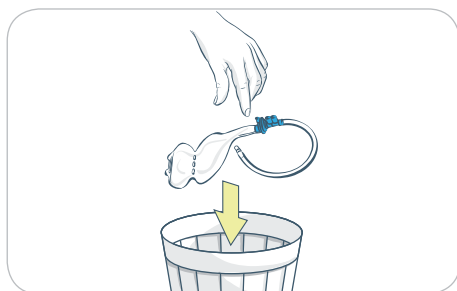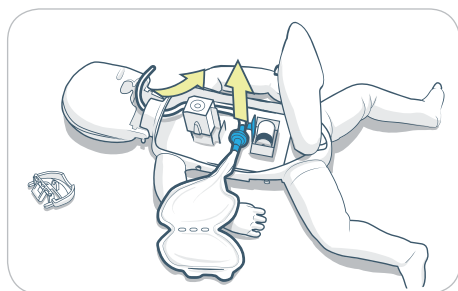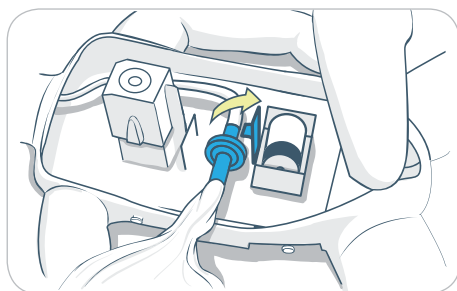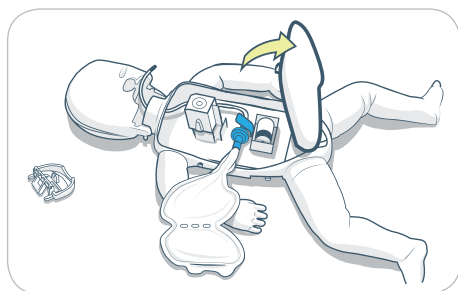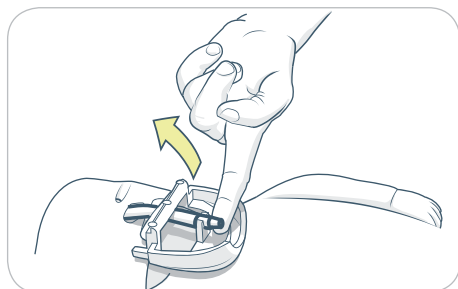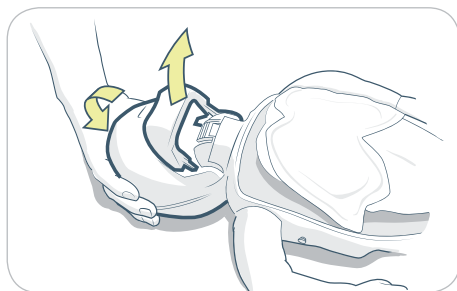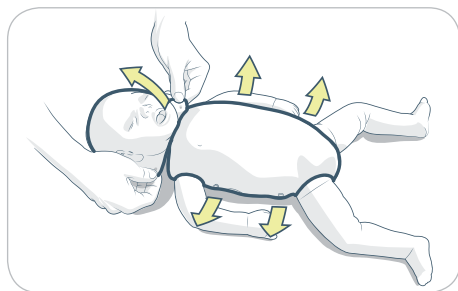

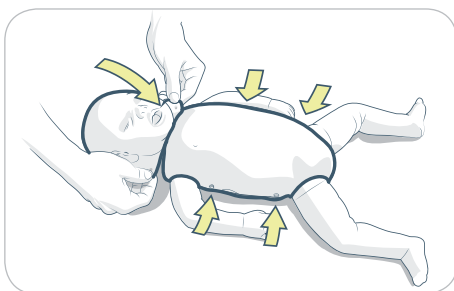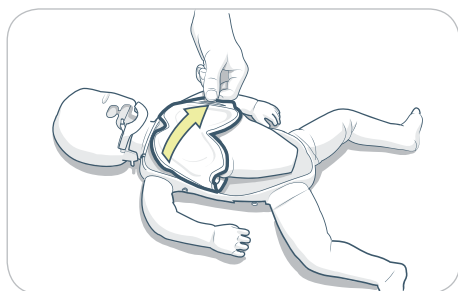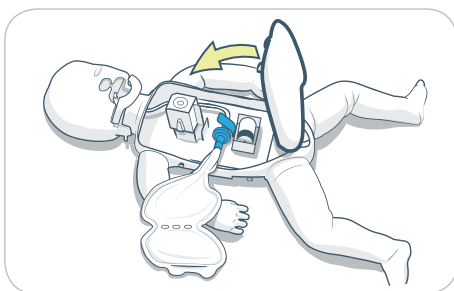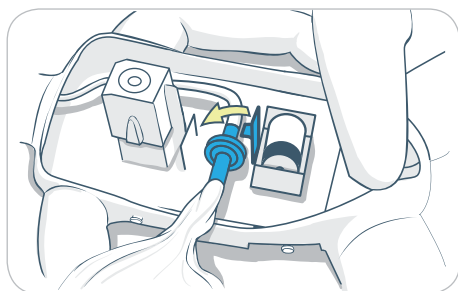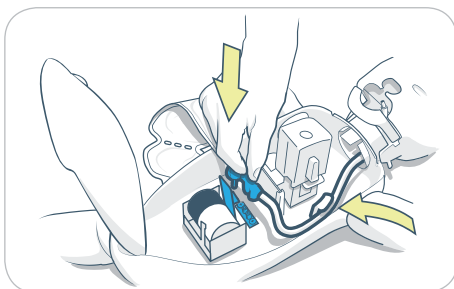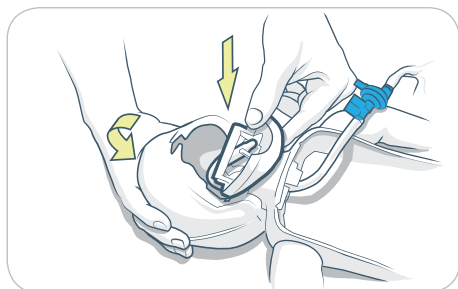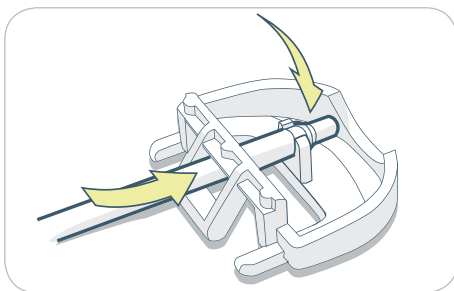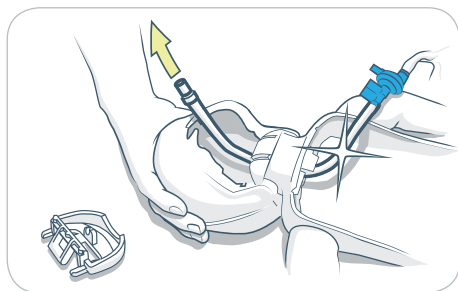

© 2013 Laerdal Medical AS. All rights reserved.
Device Manufacturer: Laerdal Medical AS, P.O. Box 377,
Tanke Svilandsgate 30, 4002 Stavanger, Norway
T: (+47) 5151 1700

20-06845 Rev A

